

# **BAYLAN**

## **WATER METERS**



### **BTB-08**

## **FULLY AUTOMATIC TEST BENCH**

Model	: BTB – 08
Nominal Diameter	: DN15 – DN25
Flowrate Range	: 8 l / h – 8 m <sup>3</sup> / h

## TABLE OF CONTENTS

1.General Information.....	2
2.Components of the Test Bench.....	4
2.1. Measuring Components .....	4
2.2.Pumps .....	7
2.3.Water Tanks.....	8
2.4.Body.....	9
2.5. Regulatory and Controlling Equipments .....	9
2.6.PLC Screen .....	11
2.7.Electrical Panel.....	12
2.8.Connection Apparatus.....	12
2.9.Compressor.....	13

### 1. General Information

The correction of the water meter is determined via calculating the errors at various flows using Baylan BTB-08 Fully Automatic Test Bench. In addition to that, whether the flow meter has a leakage under high pressures can be checked by means of the leakage test. There by, the strength of the water meter against high pressures is tested.

The movement of the piston which compresses meters is controlled by the switch located on control panel. Except the control of the switch, rest of all systems can work fully automatically.

Baylan BTB-08 Test Bench can perform tests within required flowrates for the meters between DN15 and DN25. The table below shows the quantity of the meters that can be connected to the bench in terms of nominal diameters and  $Q_3$  measuring flow rates.

***Quantity of water meters can be connected and the  $Q_3$  value of the meters according to the nominal diameters and lenghts.***

Lenght ( mm)	Pieces	Q <sub>3</sub> (m <sup>3</sup> /h)	Nominal Diameter
165	10	2,5	15
190	10	2,5	20
190	10	4,0	20
260	5	6,3	25

Baylan BTB-08 Fully Automatic Test Bench provides tests according to the directive and standards below;

<b>Recommended</b>	OIML R49 E13
<b>Standard</b>	TS EN ISO 4064 E2015
<b>Directive</b>	2014/32/EU (MID) MI-001

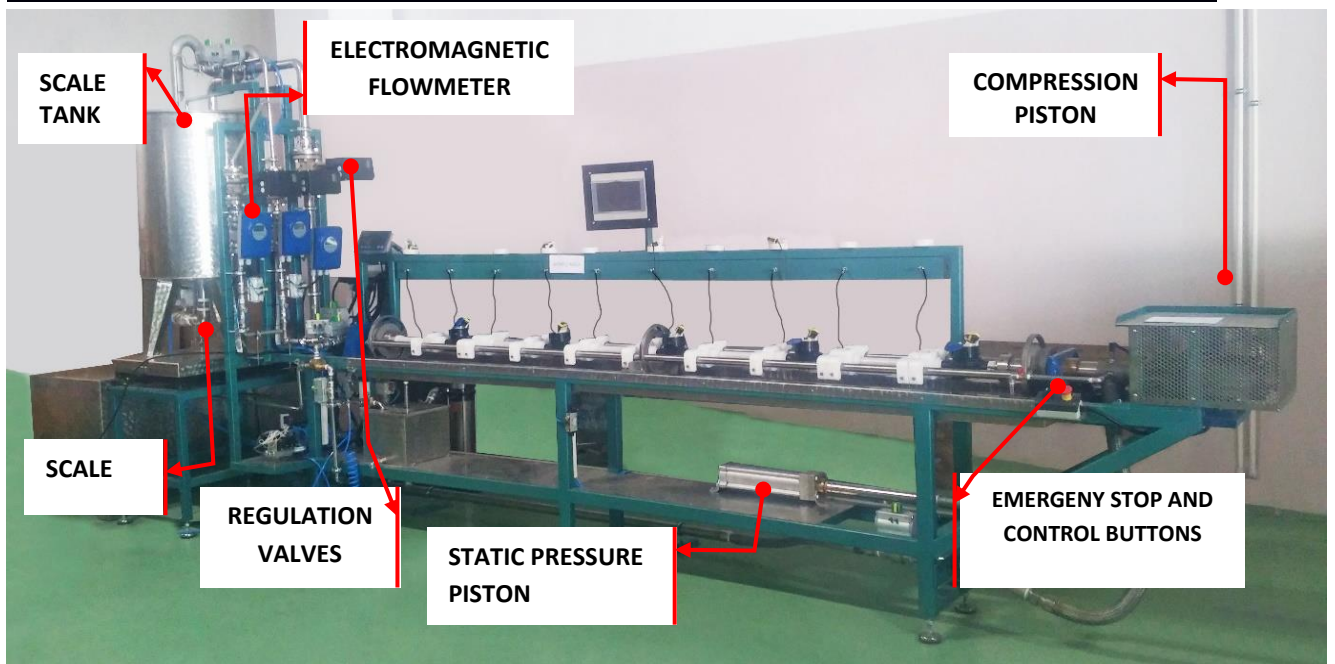


Figure 1 - Components of the Baylan Test Bench

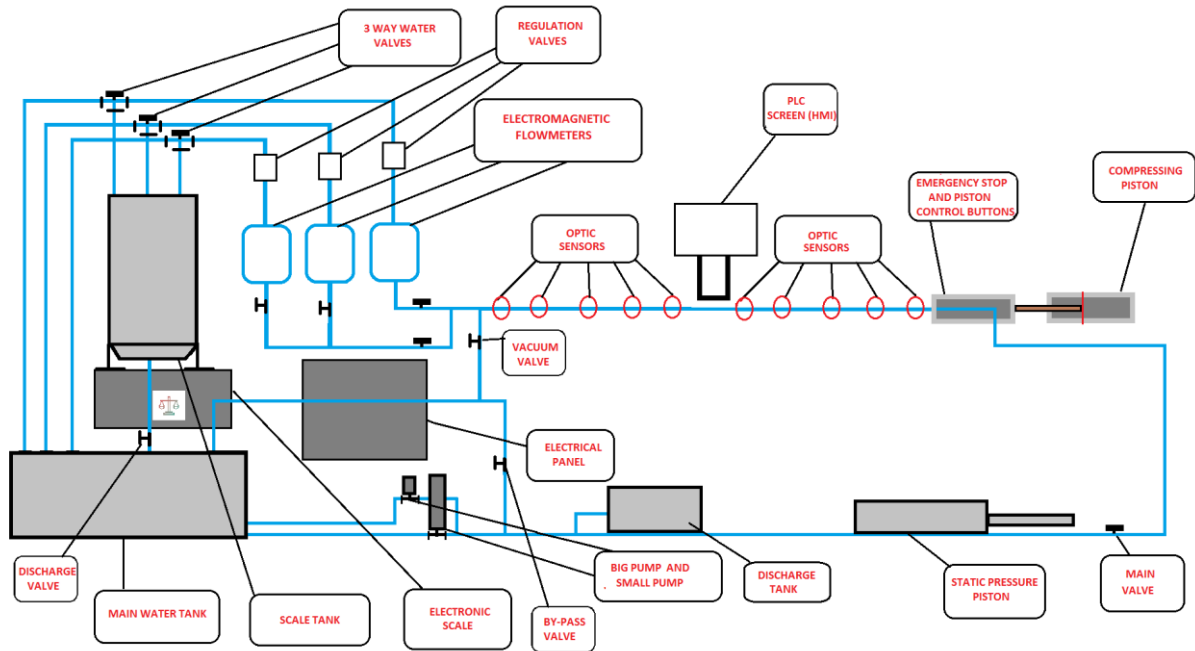


Figure 2 - Baylan BTB-08 Test Bench Chart

## 2.Components of the Test Bench

### 2.1. Measuring Components

- Flowmeter

In order to carry out the test within required flows, the flows should be stabilized at the given values. The test bench has three electromagnetic flow meters, whose measuring range is between 8 l/h – 8 m<sup>3</sup>/h . (Figure 3)

Specifications	
<b>Flowmeter Type</b>	Electromagnetic Flowmeter
<b>Electrodes</b>	Fixed Two Pairs of Hastelloy C22
<b>IP Koruması</b>	IP 66/67 EN 60529
<b>Display Screen</b>	IFC 050 Compact Model
<b>Voltage</b>	24V



Figure 3 – Flowmeter

- **Pressure Transmitter**

Pressure transmitters are located at the inlet and outlet of the test bench and they are capable of measuring pressures between 0-40 Bar. Transmitters transfer the measured data to the PLC screen and related computer.(Figure – 4)

Specifications	
<b>Measuring Range</b>	0-400 °C
<b>Temperature Sensor</b>	PT 100

Specifications	
<b>Measuring Range</b>	0-40 Bar
<b>Control Signal</b>	4-20mA



Figure 4 – Pressure Transmitter

- **Temperature Sensors**

The temperature sensors are located at the inlet and outlet of the test line of the bench. This sensors can measure between 0-400 °C. The sensors will transfer the measured temperature values to the PLC screen and to the computer in order to calculate the actual volume of the water.(Figure 5)



Figure 5 – Temperature Sensor

- **Optic Sensors**

Optic sensors are reading sensors that calculates the error curve of the meter by counting the movement of sensitive flow indicator. (Figure 6) BTB-08 Fully Automatic Test Bench is equipped with 10 sensors that can send the read data to PLC.

Specifications	
<b>Accuracy Class</b>	1
<b>Setting</b>	Manual or Automatic
<b>Output</b>	PNP ve NPN
<b>Exterior Material</b>	ABS
<b>IP Protection Class</b>	IEC IP67; NEMA 6
<b>Voltage</b>	24V



Figure 6 – Optic Sensor

- **Electronic Scale**

In order to calculate the test results and error curves, BTB-08 Fully Automatic Test Bench has a scale which can transfer datas to the related computer. The tank placed on the scale has a capacity of holding up to 250 kg of water. (Figure 7)

Scale Specifications		
<b>Measuring Range</b>	150 kg	
<b>Connection Cable</b>	2,5 meter	
<b>Pre-load Capacity</b>	64 kg	
<b>Repeatability</b>	1 g	
<b>Linearity</b>	2 g±	
<b>Sensitivity</b>	5 g	
<b>IP Class</b>	IP66	veya IP67 Cleanable Unit



## BAYLAN WATER METERS

<b>Working Principle</b>	Loadcell with Electromagnetic level balancing + IDNET converter
--------------------------	---

Scale Screen	
<b>IP Class</b>	69k
<b>Serial</b>	RS232
<b>Body Type</b>	AISI 304
<b>Screen</b>	LCD Crystal Screen

Figure 7 – Electronic Scale Screen

## 2.2.Pumps

BTB-08 Fully Automatic Test Bench has 2 different pumps working separately for high and low flowrates. In order to provide clean water passage between the tanks and the pumps, closing valves and control valves are equipped with filters.

- **Big Pump**

For the flowrates higher than 0,5m<sup>3</sup>/h.

Big Pump Specifications	
<b>Control Type</b>	Frequency Controlled
<b>Working Principle</b>	Centrifuge
<b>Obtainable Working Pressure</b>	11 bar
<b>Maximum Flowrate</b>	16m <sup>3</sup> /h (*)



Figure 8 – Small and Big Pump

- **Small Pump**

For the flowrates lower than 0,5m<sup>3</sup>.

Small Pump Specifications	
<b>Control Type</b>	Frequency Controlled
<b>Obtainable Working Pressure</b>	5 bar

(\*) NOTE: Maximum flow rate of the pumps can change with the water meters quantity, magnitude and pipes inner circle diameters.

Specifications of Water Tanks	
<b>Maximum Flowrate</b>	0,5 m <sup>3</sup> /h (*)
<b>Material</b>	AISI 304 Stainless Steel
<b>Capacity</b>	20 liter
<b>Scale Tank</b>	250 liter
<b>Discharge Tank</b>	12 liter

## 2.3. Water Tanks

- Main Water Tank

Main water tank is a tank that where all the water is collected after the measurement of the water mass. In order to prevent any overflow, the appendent water-gauge inside of the tank sends order to the system to stop water flow.



*Figure 9 – Main Water Tank*

- Scale Tank

Scale tank is the tank that measures and collects the weight of water that water meters passes through within the testing process. If the weight is over the capacity of the tank the PLC system will shut down the inlet valve and in addition to this discharging valve will start working in order to discharge the water from scale tank to main tank. Besides, water-gauge which located inside of the scale tank, does the same job as flooding security.



*Figure 10 – Scale Tank*

- Discharge Tank

In the process of mounting and dismounting meters to the test line, discharging tank holds the water . By the submerge pump , water will be transferred from discharge tank to the main water tank. Also there is valve added for evacuation.

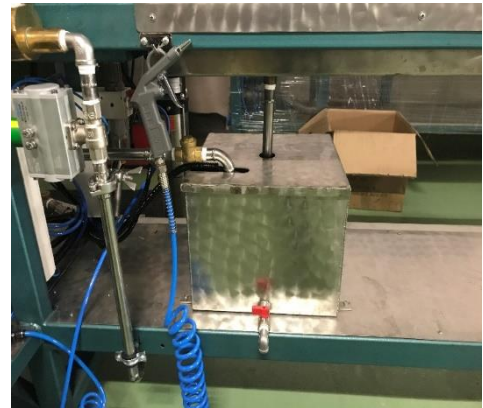


Figure 11 – Discharge Tank

## 2.4.Body

It's a construction that gathers the components of the test bench. It's made of steel covered with stainless sheet. It is ergonomically designed for easy use.

## 2.5. Regulatory and Controlling Equipments

- Compression Piston


Meters which will be mounted to the test line are stabled by the pneumatic piston. Within this system there is security valve and non-return valve. System is controlled by the rotative key. To make sure compression process is complete, user should control the arrows that shows compressor piston accuracy on the PLC screen. The system, will not start testing, vacuuming or apply pressure until the



Specifications	
<b>Material Type</b>	ST-37
<b>Paint Type</b>	Epoxy

compression piston fully compresses the test line.

Figure 13- Compression Piston

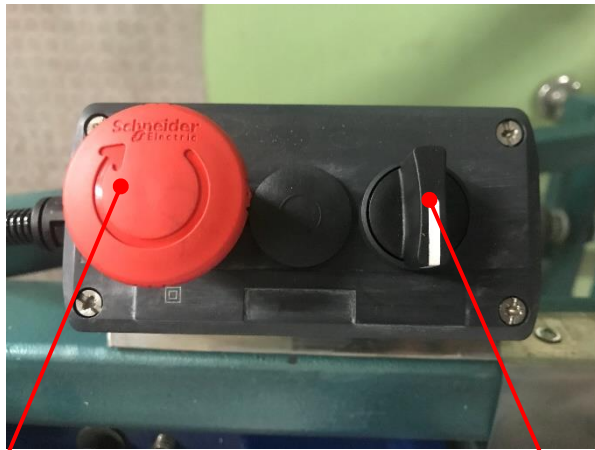

**Rotative Key ( Switch ):**

Switch makes compressor piston goes forward and backwards. The piston will move to the direction where switch is rotated.

Emergency Stop Button      Emergency Stop Button      Rotative Key

Figure 14 –Rotative Key and

- **Static Pressure Piston**

While applying the static pressure test, required pressured air is manually set by use of pneumatic pressure adjuster by the operator. (Figure 14) If the pneumatic adjuster moves down, pressure raises up and if it moves up it releases the pressure. (Figure 15)



Figure 14 – Static Pressure Piston

Figure 15 - Pneumatic Pressure Adjuster

- **Regulator Valves**

Baylan BTB-08 Fully automatic test bench has three different regulator valves and three different flow meters which control the flowrates between 8 l/h–8 m<sup>3</sup>/h.



Figure 16 - Regulator Valves      Figure 17

Specifications	
<b>Valve Type</b>	Engined, 2 ways pneumatic valve
<b>KVS</b>	0,25      1,6      10
<b>Material</b>	Stainless Steel

<b>Working Range</b>	-10 / 220 C
<b>Flow Characteristic</b>	Evenly
<b>Engine Type</b>	Electrical Motor 3374-15
<b>Voltage</b>	24V
<b>Control Signal</b>	4-20mA

- **Pneumatic Valves**

Pneumatic controlled spherical valves controls the water flow. Movement of the spherical valves is provided by the parameters that has entered before.

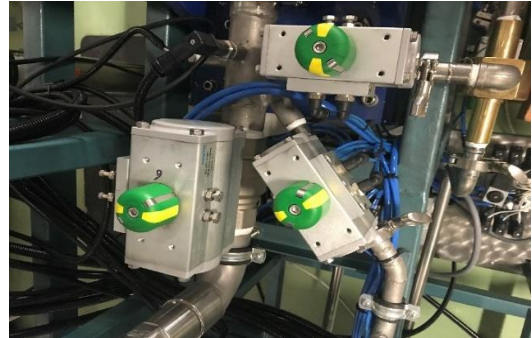


Figure 18 – Pneumatic Valves

**Main Valve:** The main valve is which starts the water flow at the test bench.

**Discharge Valve:** Discharge valves are which provides the water inside of scale tank evacuates to main tank.

**Vacuum Valve:** Vacuum valve is the valve that which provides connection between main line and vacuum line. By this way it is used for vacuuming air.

**By-Pass Valve:** By-pass valve is used for creating circulation for vacuuming.

**Three way valves:** Three way valve allow flow coming water from the meters to water tank or scale tank.

## 2.6.PLC Screen

Through the PLC screen, error curves of the meters and the results can be displayed. Besides, the system and testing process can be control by using touchscreen. In terms of rotatability of the PLC screen, it is mounted to the test bench’s body and it can be positioned as required.

Specifications	
<b>Screen Size</b>	10”
<b>Screen Type</b>	Color Screen
<b>Input Mode</b>	Touch Screen
<b>Connection Type</b>	USB + Ethernet + RS32 + RS 488

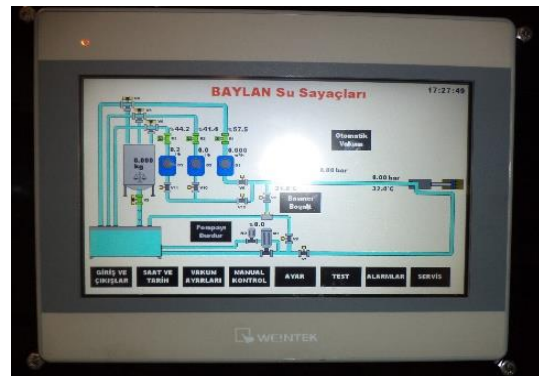


Figure 18 – PLC Screen

## 2.7. Electrical Panel

Electrical panel which located on the test bench has PLC command unit, power source ( 24 V), frequency control unit which set the motors rotation of pumps, electrical switches which run the devices that operates with electric.

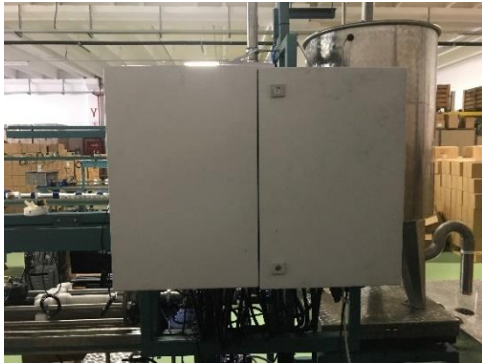


Figure 19

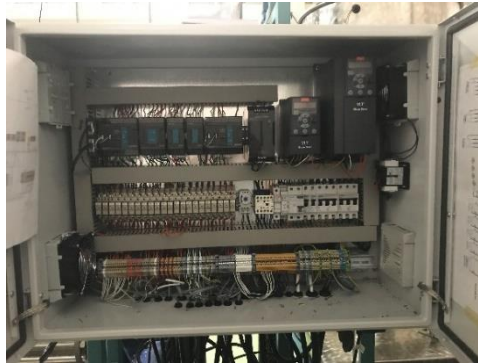


Figure 20

Figure 19 - Electrical Panel - Figure 20

## 2.8. Connection Apparatus

Before the test begins, in order to mount meters to the connection line, between every single meters and also at the inlet and outlet of connection line, there should be apparatus made of POM. POM apparatus are durable against strikes and breakage. Also, POM apparatus made from the same material with the support apparatus for stabilizing the water meters to the test bench.



Figure 20 – POM Connection Apparatus



Figure 21 – Support Apparatus

Specifications	
Material Type	POM
Nominal Diameter / Meter Length	DN15 / 170mm
Nominal Diameter / Meter Length	DN20 / 190mm
Nominal Diameter / Meter Length	DN25 / 260mm

## 2.9.Compressor

Test panel system requires compressed air. The compressor provides this compressed air requirement. Compressor is powered by single-phase electric line and operating voltage is 220V in this test bench.

Specifications	
<b>Air Pressure (Minimum)</b>	6 bar
<b>Air Tank Capacity</b>	50 litre
<b>Voltage</b>	220 V



Figure 22 – Compressor